



# FluoroQuant® Afla Test Method


## Detects aflatoxin in decorticated cottonseed and cottonseed meal

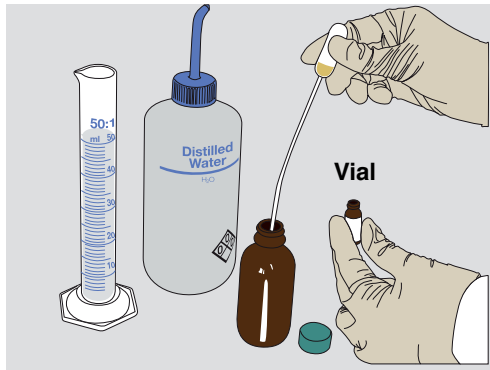


- 1) Prepare developer by adding contents from 1 vial to 25 mL distilled water, (make fresh after 8 hours).

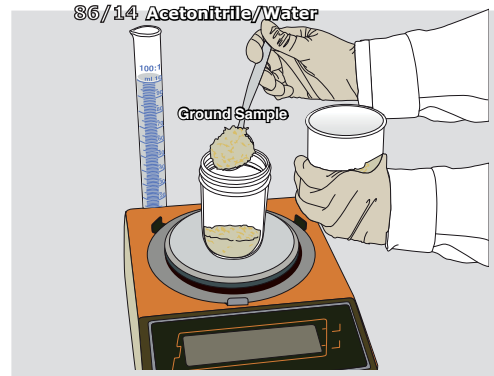


- 2) Weigh 5g ground sample and add to 20mL 86/14 acetonitrile/water, vortex for 3 minutes, & filter.

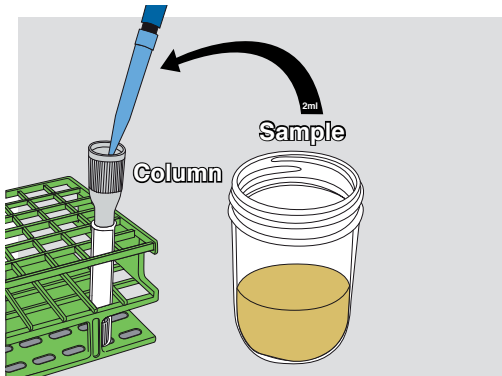

- 3) Place 2mL (2000µL) sample extract into top of column.

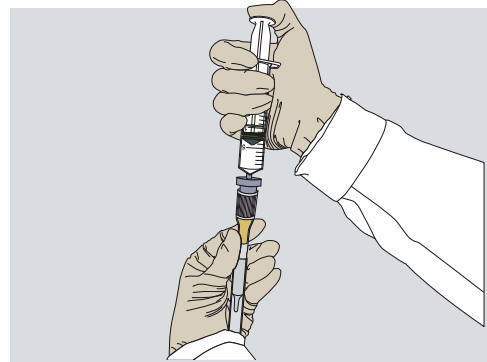

- 4) Remove tip, place column in cuvette, insert syringe plunger into column and push extract thru column slowly (30-40 sec.)

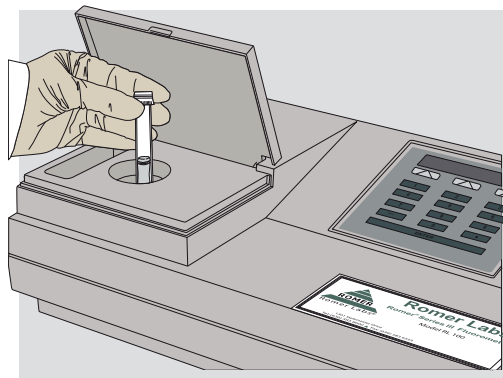

- 5) Transfer 1mL (1000µL) of extract to clean cuvette, add 1mL of developer, cap, vortex, wipe cuvette with lint-free paper and read after 30 second delay.