



AgraVision™ Quick Guide for application with AgraStrip® Mycotoxin tests


1. Switch ON the AgraVision™ Reader by pressing the Power button at the rear of the instrument.
2. Select „TEST“

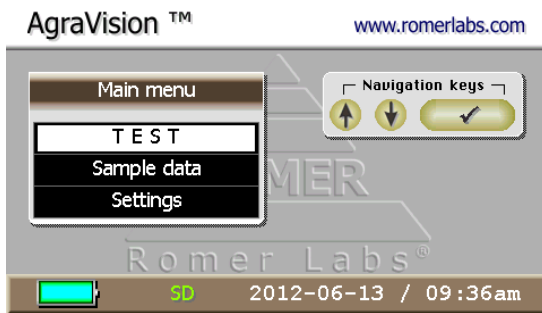

3. Select the designated Analyte (Mycotoxin)

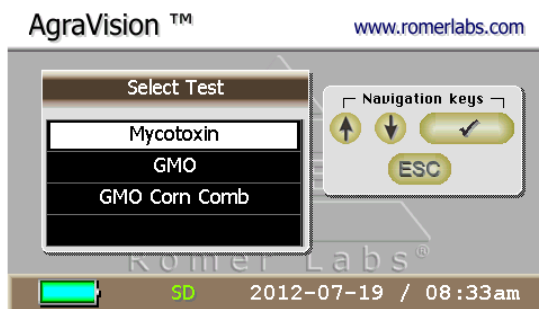


4. By pressing ↑ and ↓ move the flashing cursor to the strip position that corresponds to the position of the strip inserted into the tray.

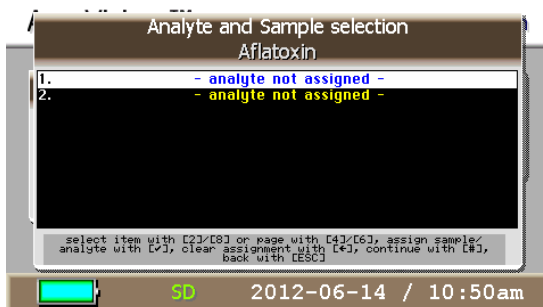


5. Now scan the correct barcode (matrix dependent) either from AgraStrip tube or from the certificate of performance. A beep sound will signal successful scanning.

- A new window will open requesting a "Sample ID". Either key in a sample ID, scan a sample ID bar code or select from the menu listed on the screen. For selection of existing sample IDs press "#" and then press the "↓" key multiple times until you reach your designated sample ID.

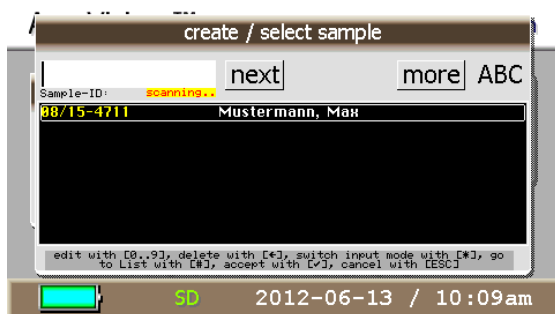

- Assign the next strip position according to steps 4., 5. and 6. or press the "#" key to skip the next tray position.
- Now enter the operator information. This can be done by keying in an operator name/ID, scanning an operator ID bar code or selecting from the listed operators on the screen. For selection of existing operators press "#" and then press the "↓" key multiple times until you reach your designated operator.

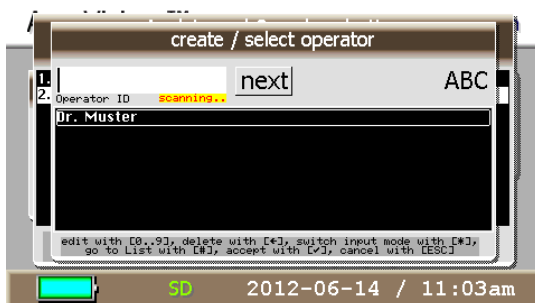

- Insert the mycotoxin tray with developed test strips and press the "✓" key to start the measurement.
- Results will be displayed after less than 10 seconds.

